DRAWING # 61

MANUAL RETRACTABLE CEILING COLUMN

(M/N: C-COL-MANU)

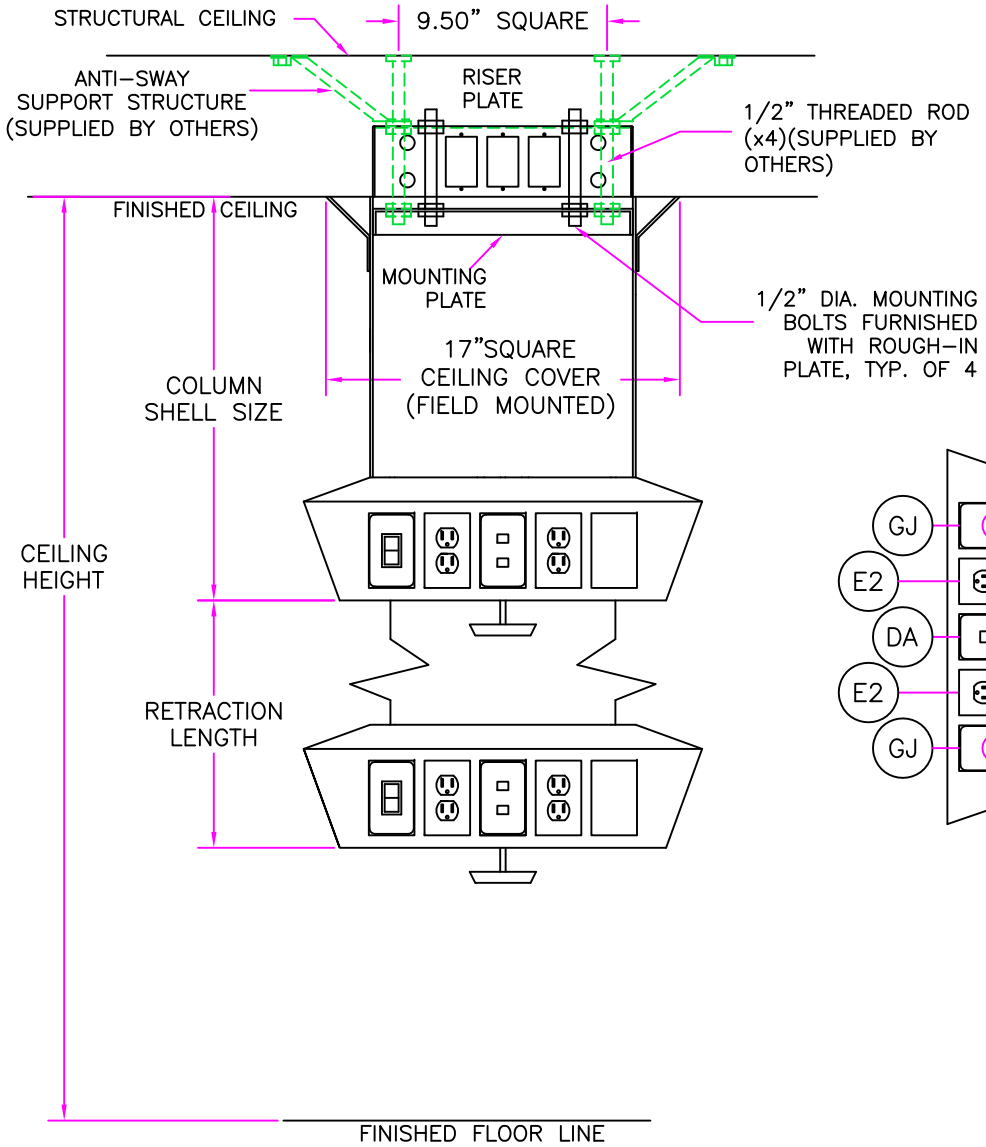

TYPE:

QUANTITY:

SYSTEM DETAILS		
SYMBOL	QTY.	DESCRIPTION
CC	1	CEILING COLUMN
E2	6	RECEPTACLE - DUPLEX RED
DA	3	PROVISION - DATA
GJ	2	GROUND JACK
2	1	GAS, NITROUS OXIDE
N	1	GAS, NITROGEN
W	1	GAS, WAGD
O	2	GAS, OXYGEN
A	2	GAS, MED AIR
V	2	GAS, VACUUM
NCP	1	NITROGEN CONTROL PANEL

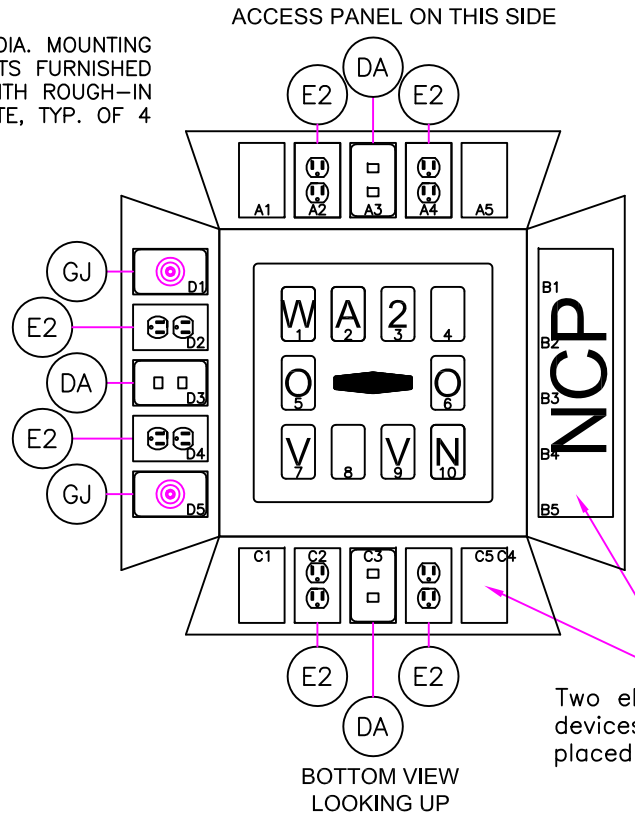

Two electrical/communication devices or gases cannot be placed toghether at any corner.

AMICO CORPORATION
01/01/08
FOR PRESENTATION PURPOSES ONLY

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE _____ DATE _____ PHONE NO. _____

AMICO Corporation
85 Fulton Way
Richmond Hill, Ontario
L4B 2N4, CANADA
Toll-Free: 1-877-462-6426(T)
1-866-440-4986(F)
Tel: (905) 764-0800
Fax: (905) 764-0862
www.amico.com

HOSPITAL	HOSPITAL	A. NURSE CALL MFGR: _____ MODEL NO.: _____	DRWG. NO.
LOCATION	LOCATION	B. MEDICAL GAS MFGR.: _____ TYPE CONNECTION: _____	PRICEBOOK–62
QTY. 1		C. FINISH: _____ CEILING HEIGHT: _____	DRAWN BY:CS
			CHECKED BY:CS
			REV.NO.:
			DATE: