DRAWING # 63

# MOTORIZED RETRACTABLE CEILING COLUMN

(M/N: C-COL-ELEC)




TYPE:

QUANTITY:

| SYSTEM DETAILS | | |
|---|---|---|
| SYMBOL | QTY. | DESCRIPTION |
| CC | 1 | CEILING COLUMN |
| E2 | 6 | RECEPTACLE - DUPLEX RED |
| DA | 1 | PROVISION - DATA |
| MT | 1 | MOTORIZED UP/DOWN SWITCH |
| 2 | 1 | GAS, NITROUS OXIDE |
| E | 1 | GAS, EVAC |
| O | 2 | GAS, OXYGEN |
| A | 2 | GAS, MED AIR |
| V | 2 | GAS, VACUUM |

ACCESS PANEL ON THIS SIDE

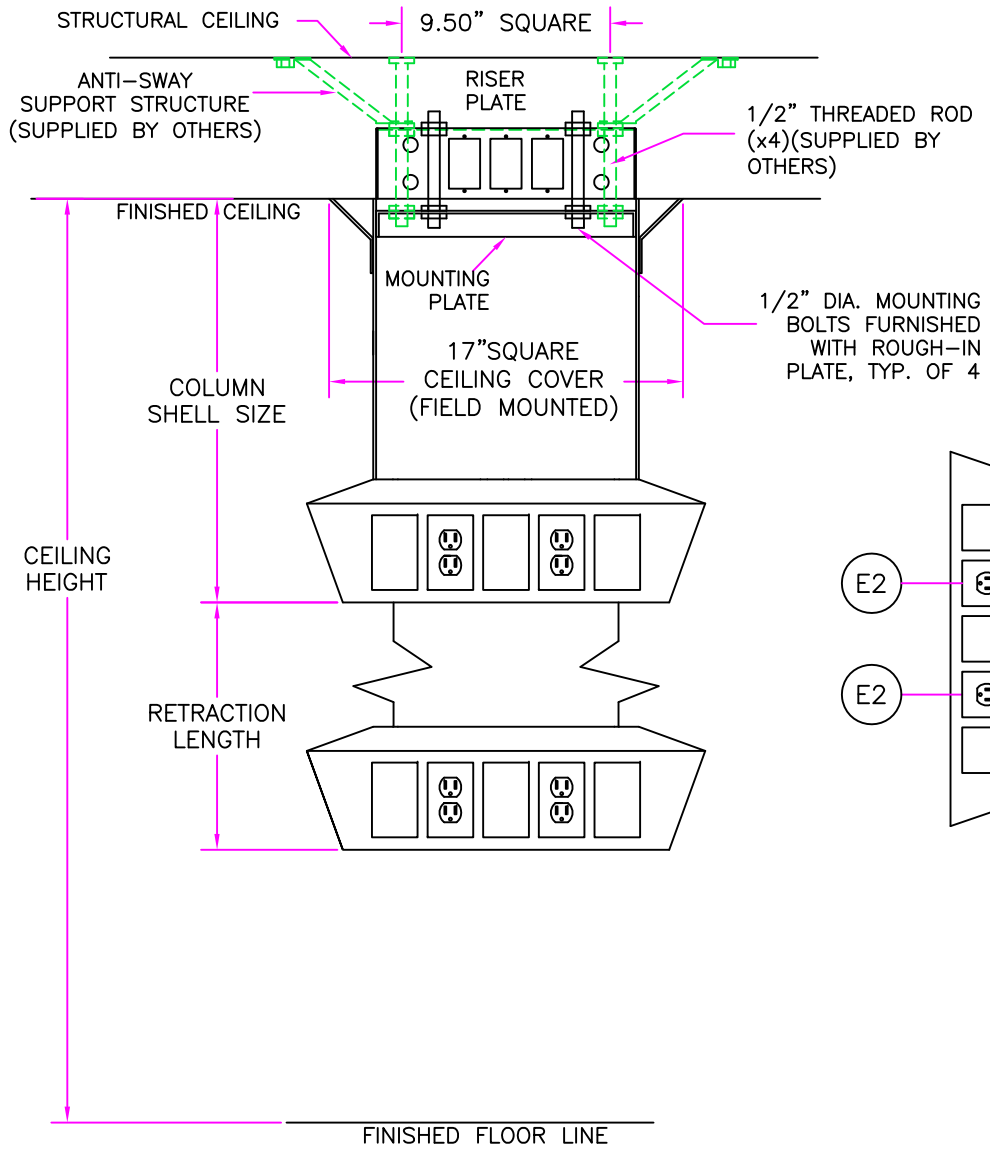


BOTTOM VIEW LOOKING UP

Two electrical/communication devices or gases cannot be placed toghether at any corner.

AMICO CORPORATION 01/01/08 FOR PRESENTATION PURPOSES ONLY

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

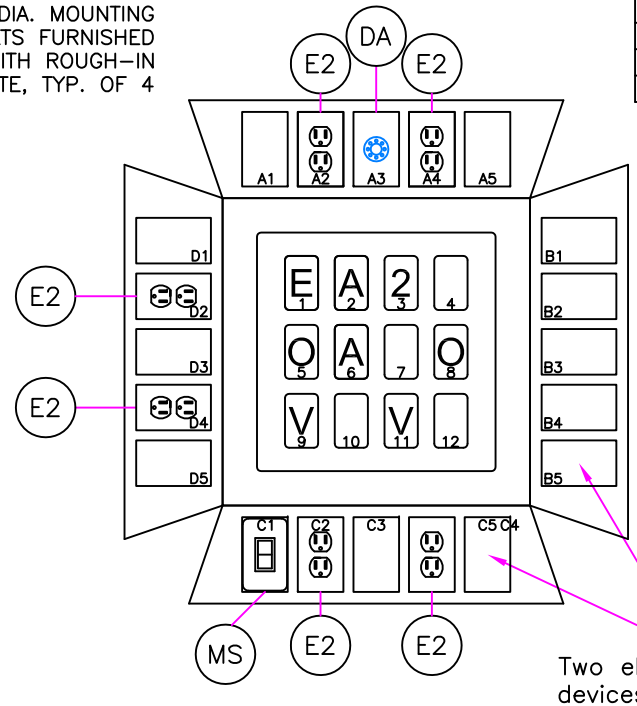APPROVAL - PRINT AND SIGNATURE _____ DATE _____ PHONE NO. _____


AMICO Corporation
85 Fulton Way
Richmond Hill, Ontario
L4B 2N4, CANADA
Toll-Free: 1-877-462-6426(T)
1-866-440-4986(F)
Tel: (905) 764-0800
Fax: (905) 764-0862
www.amico.com


| | | | |
|---|---|---|---|
| HOSPITAL | HOSPITAL | A. NURSE CALL MFGR: _____ MODEL NO.: _____ | DRWG. NO. |
| LOCATION | LOCATION | B. MEDICAL GAS MFGR.: _____ TYPE CONNECTION: _____ | PRICEBOOK–66 |
| QTY. 1 | | C. FINISH: _____ CEILING HEIGHT: _____ | DRAWN BY:CS |
| | | | CHECKED BY:CS |
| | | | REV.NO.: |
| | | | DATE: |